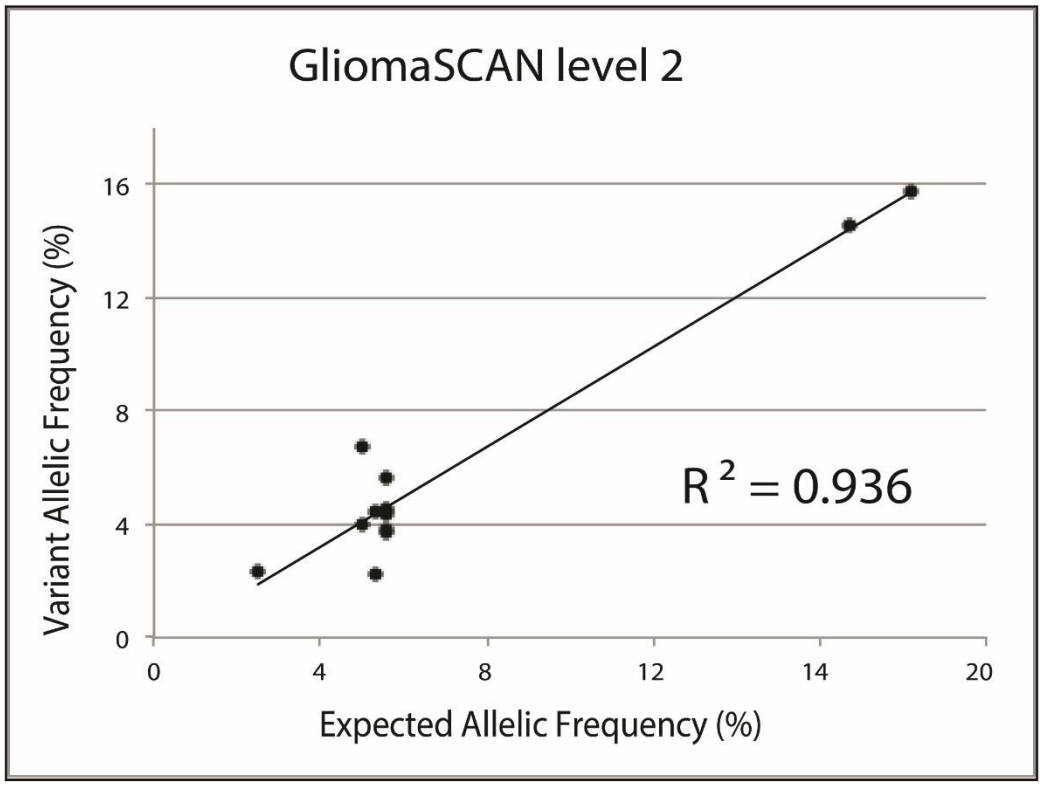

S6 Fig. Correlation analysis of expected allelic frequency with measured allelic frequency in Horizon HD753.